



Recommended power specifications for mobile CT

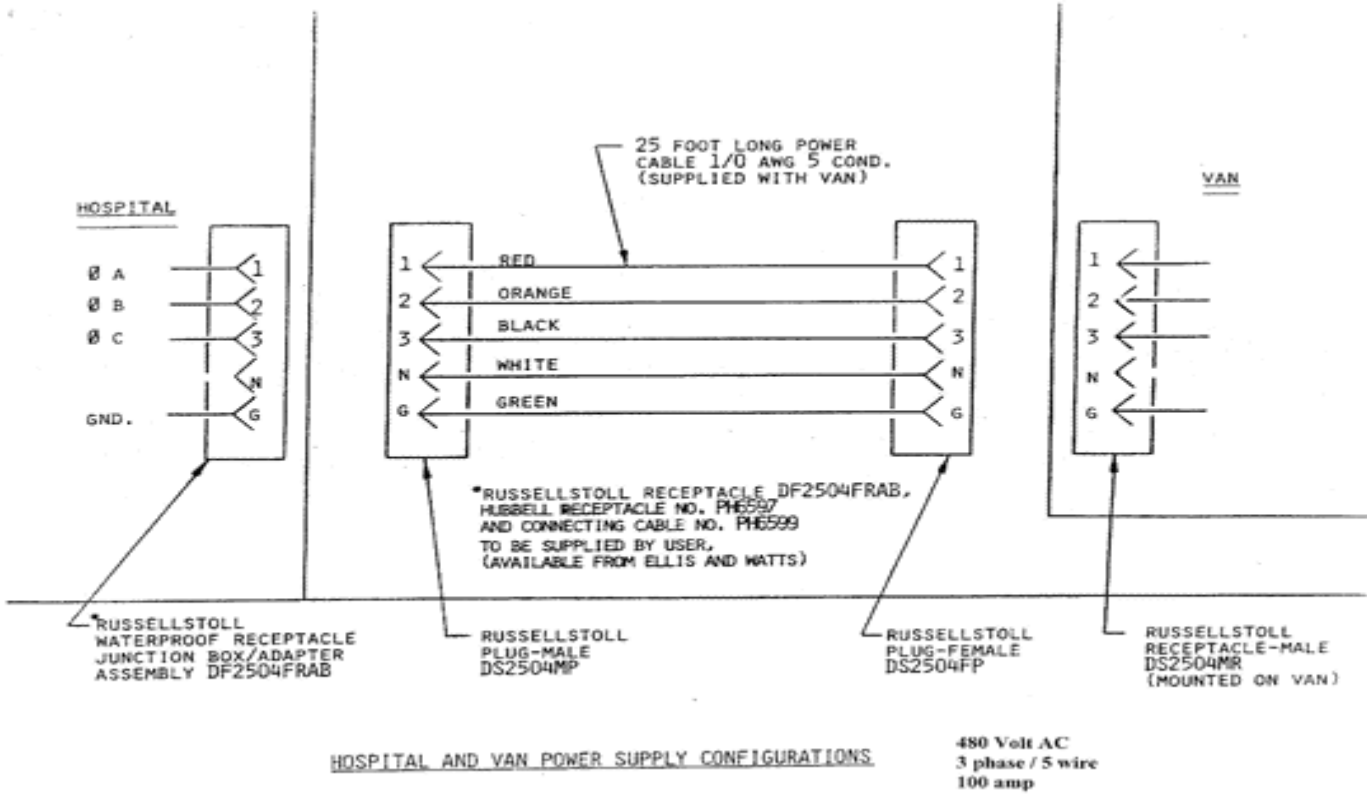

Minimum 150 Amp service needed as of January 1, 2006.  
Neutral not needed

Cat 5 cable only needed if they want to connect to a network

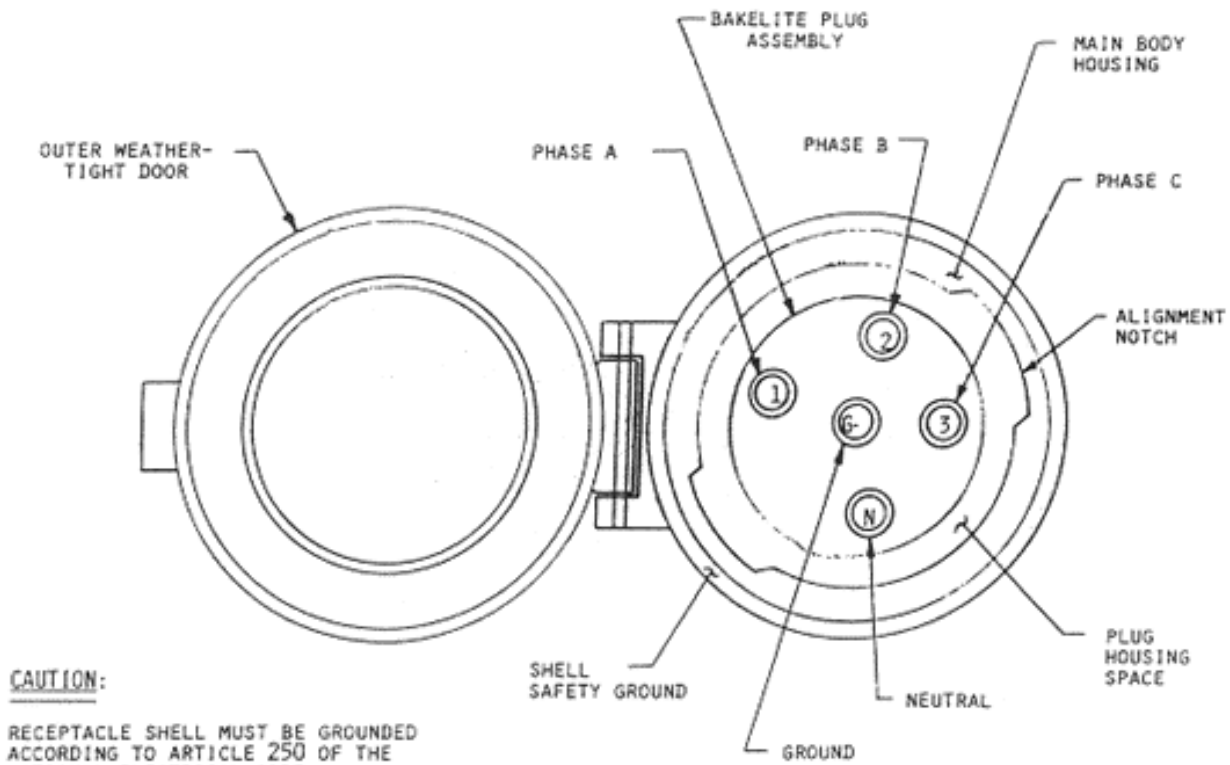

CAUTION:

RECEPTACLE SHELL MUST BE GROUNDED  
ACCORDING TO ARTICLE 250 OF THE  
NATIONAL ELECTRICAL CODE.

RUSSELLSTOLL #DF2504FRAB

HOSPITAL RECEPTACLE WIRING CONFIGURATION



FROM DBRS MOBILE



SHORE POWER FROM FACILITY

